

Digital Sound Level Meter Operation manual



Version: A0

A. Introduction

This equipment has been designed to meet the measurement requirement of Safety Engineers, Health, Industrial Safety offices and Sound Quality control in various environment, which include factory, office, traffic, family, and audio system.

This equipment has the following functions:

1. It is designed according to the IEC651 TYPE2 & ANSI S1.4 TYPE2
2. Accuracy up to +/- 1.5 dB
3. Measurement range: 30-130 dB
4. With two equivalent weighted sound pressure levels, A and C.
5. Fast & Slow dynamic characteristic modes.
6. AC and DC output for frequency analyzer level recorder, FFT analyzer, graphic recorder etc.

B. Safety Notice

Operation Environmental condition:

1. Below 2000 meters in height;
2. Operation humidity: 10~80%RH
3. Operation temperature: 0~40°C

Maintenance:

Use dry cloth to clean the unit, but never with any solvent.




Figure1

B. Calibration Procedures:

Please use a Standard Acoustic Calibrator.

1. Make the following settings:
Equivalent weight: A Time weight: FAST
Level range: 60 to 110 dB
Measurement mode: MAX function disable

2. Insert the microphone carefully into the 1/2 inch hole of the Calibrator.
3. Turn on the Calibrator and adjust the Potentiometer inside the battery compartment of the unit (shown in the Figure 1), until the LCD display the desired Level 94.0dB.

**Our products are all well calibrated before Shipment.
Recommended recalibration cycle: 1 year.

D. Name and functions (Figure 2)

1. Electret Condenser Microphone.
2. LCD Display.
3. Power switch
4. Level range control switch:
30dB~80dB; 50dB~100dB; 60dB~110dB;
80dB~130dB; 30~130dB
5. Maximum value hold switch. (MAX)
6. Equivalent weight select switch:
A: A weight for general sound level measurements.
C: C weight for checking the low frequency content of noise.

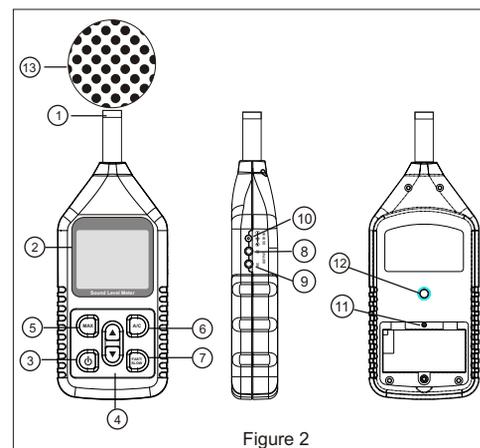


Figure 2

7. Time weight select switch:
Fast: For normal measurements.
Slow: For checking average level of fluctuating noise.
8. AC output terminal: 0.707 Vrms Corresponding to each range step.
9. DC out put terminal: output 10 mV/ dB
10. External DC 6V power supply terminal.
11. Calibration control
12. Tripod mounting screw.
13. Windscreen.

F. Pre-operations:

1. Open the battery door and insert 9V battery into the battery compartment.
2. Cover the battery door.
3. When the battery voltage drops below the operating Voltage, mark "□" appears. Replaced with a new battery
4. When the DC adapter is used, insert the plugs (3.5 φ) of the adapter into the DC 6V connector.

H. Caution

1. Do not operate the unit at high temperature and Humidity environment.
2. Please take out battery from unit if not in use for any extended period of time.
3. Once using the unit in the presence of wind, it is must to mount the windsreen to make sure not pick up undesired signals.

E. LCD Display (Figure 3)

1. Level range.
2. Under range.
3. Low battery indication.
4. Maximum value is held during measuring.
5. Measuring value.
6. Measuring Unit.
7. Frequency weight A/C.
8. Bar graph.
9. Over range.
10. Slow time weight.
11. Fast time weight.

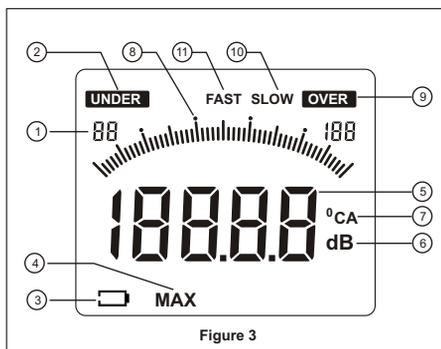


Figure 3

G. Operation

1. Turn on the unit.
2. Select the desired measuring range until the LCD not display "Under" or "Over"
3. If measure general noise sound level, please select dBA.
4. If the sound source consists of the short bursts of only catching sound peak, set response to FAST. To measure average sound level, set response to slow.
5. When MAX mode is chosen. The instrument hold the maximum noise level.

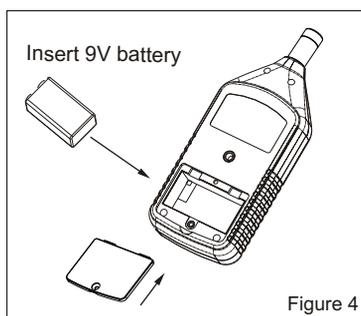


Figure 4

I. Specification

| | |
|-----------------------|--|
| Measuring range | 30~130dBA, 35~130dBC |
| Accuracy | +/- 1.5 dB (under reference conditions) |
| Frequency range | 31.5Hz-8.5KHz |
| Level range | 30-80,50-100,60-110,80-130, 30~130dB |
| Linearity range | 50dB / 100dB |
| Frequency weighting | A / C |
| Digital Display | 4digits |
| Resolution | 0.1dB |
| Sample rate | 2 times/second |
| Bar graph | 50 dB scale at 1 dB step for monitoring current sound pressure level display Sample rate: 2times/second |
| Over indication | OVER / UNDER |
| AC output | 0.707Vrms at FS output impedance approx. 600 ohm |
| DC output | 10mV/dB, output impedance approx. 100ohm |
| Time weight | FAST / SLOW |
| Microphone | 1/2 inch electret condenser microphone |
| Max | MAX |
| Power supply | 9V battery |
| Power life | About 30 hours (alkaline battery) |
| Self calibration time | 3 s |
| Operating condition | 0~40°C, 10~80%RH |
| Storage condition | -10~60°C, 10~70%RH |
| Weight | 230g (including battery) |
| Dimension | 207*70*29mm |



MADE IN CHINA